


Supplementary Materials

Measurement of SARS-CoV-2-binding human IgG using the EUROIMMUN test.

The amounts of SARS-CoV-2-binding human IgG in the serum sample were measured with Anti-SARS-CoV-2 (anti-S1) ELISA (IgG) (EUROIMMUN AG, Lübeck, Germany), a commercial enzyme-linked immunosorbent assay, according to the manufacturer's instructions. Results with an optical density (OD_{450nm}) ≥ 0.497 were regarded as seropositive.

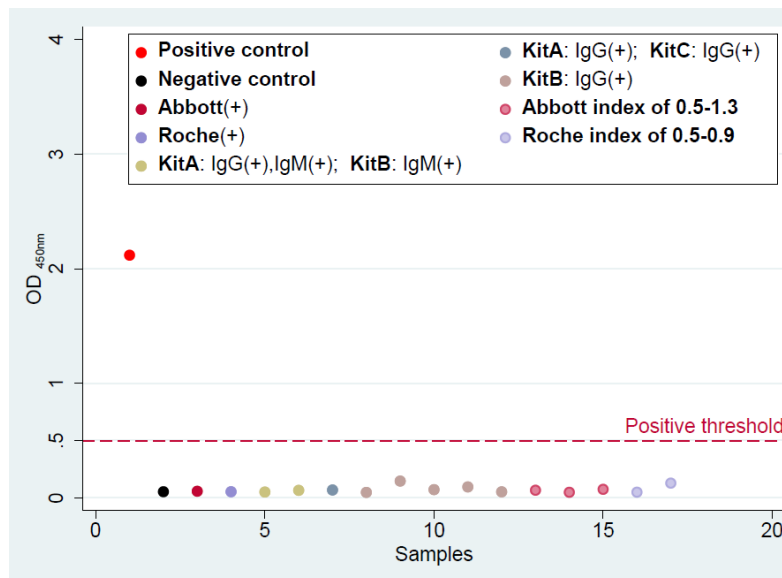

Supplementary Figure S1. Individual values of the EUROIMMUN test (IgG) in a convenience selection of samples.

The Y-axis shows the optical density (OD_{450nm}). The X-axis shows the results of the positive control, negative control, and 15 individuals who were positive on Abbott, Roche, Kit B (IgG), two or more kits, and those with Abbott index of 0.5-1.3 or Roche index of 0.5-0.9.

(+): positive

The positive threshold value is 0.497.